



U2™ Revision Stem

Revision Femoral Hip System



U2 Revision Stem –

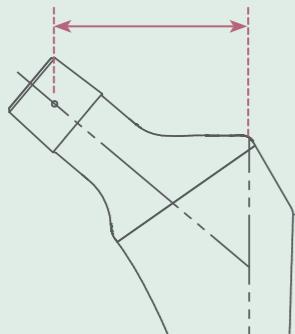
The U2 Revision Stem is a monoblock fully Titanium Plasma Spray (TPS) coated cylindrical stem optimized for revision hip arthroplasty.

The design rationale of the U2 Revision Stem is based on primary U2 Hip Stem. It shares in the same geometrical neck concept and also utilizes the tri-wedge geometry to achieve implant stability, similar to the primary system. However, the revision system offers a shorter neck offset design than the primary system to help facilitate joint reduction in revision patients. 180 mm and 230 mm stem length options with Ø11 mm to Ø18 mm distal diameter are available to allow for treatment of patients with bone deficiency and anatomy variations.

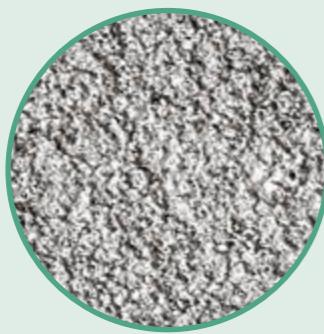


U2 Revision Stem Offset Length

- 3~5 mm shorter than U2 hip stem

**Shorter Offset Than Primary Implant Designs**

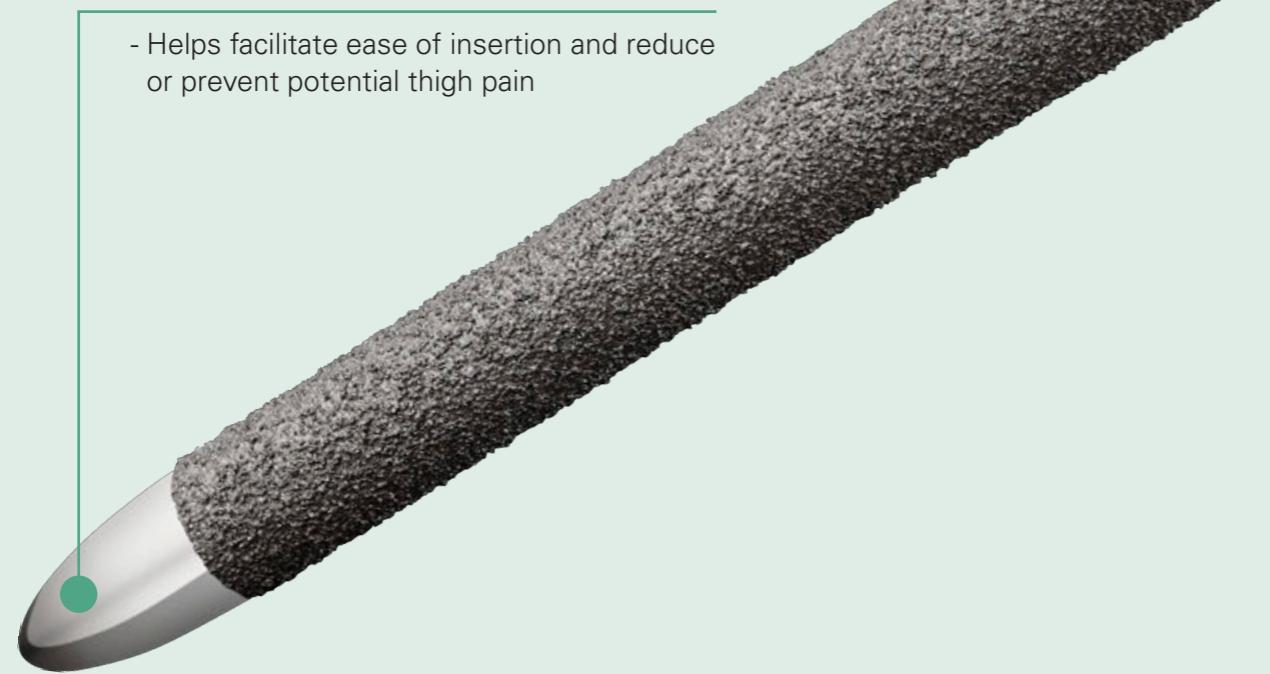
- Facilitate joint reduction for patients with soft tissue scarring or contracture from previous surgeries

**Fully Titanium Plasma Spray Coating**

- Designed to promote biological fixation

Polished Bullet Tip

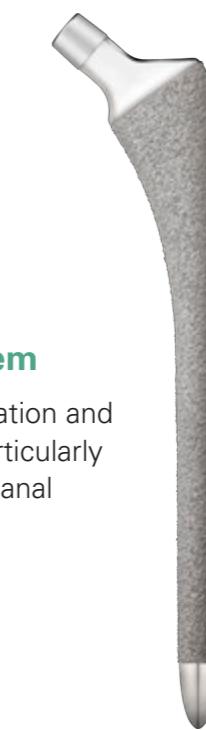
- Helps facilitate ease of insertion and reduce or prevent potential thigh pain

**12/14 Neck Taper**


- Accommodates a complete selection of femoral heads

Proximal Tri-Wedge

- Designed to provide rotational and axial stability

**Straight 180 mm Length Stem**

- Designed to enable diaphyseal fixation and avoid the risk of bone fracture, particularly for patients with a small femoral canal

**Curved 230 mm Length Stem**

- Designed to fit the anatomical shape of a femoral canal with increased bone deficiency and prevent potential cortical impingement and intraoperative shaft fracture

Anterior Bowing

Order Information



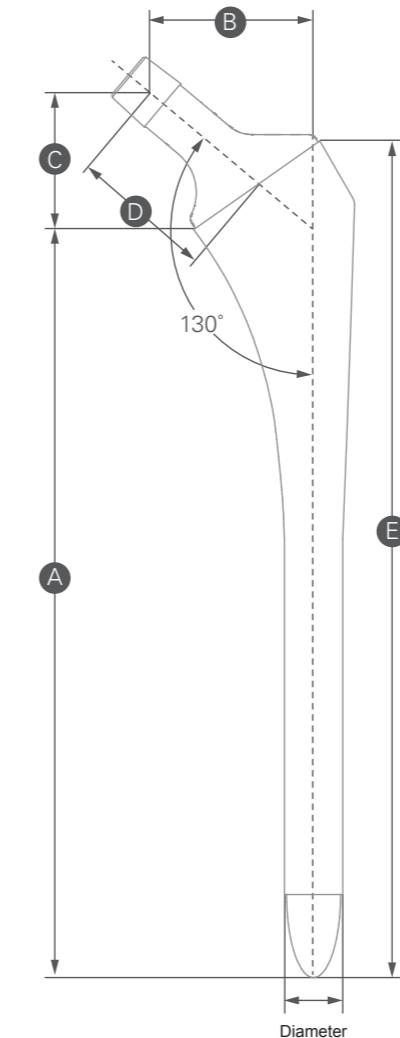
Catalog Number	Description
----------------	-------------

U2 Revision Stem
Straight

1104 - 1611	$\varnothing 11$
1104 - 1612	$\varnothing 12$
1104 - 1613	$\varnothing 13$
1104 - 1614	$\varnothing 14$
1104 - 1615	$\varnothing 15$
1104 - 1616	$\varnothing 16.5$
1104 - 1618	$\varnothing 18$

Curved

Left	Right	Diameter
1104 - 1711	1104 - 1811	$\varnothing 11$
1104 - 1712	1104 - 1812	$\varnothing 12$
1104 - 1713	1104 - 1813	$\varnothing 13$
1104 - 1714	1104 - 1814	$\varnothing 14$
1104 - 1715	1104 - 1815	$\varnothing 15$
1104 - 1716	1104 - 1816	$\varnothing 16.5$
1104 - 1718	1104 - 1818	$\varnothing 18$



Diameter	A Medial Length	B Offset	C Vertical Height	D Neck Length	E Lateral Length
Straight					
$\varnothing 11$	180	35	24.6	27	199
$\varnothing 12$	180	35	25.6	27	200
$\varnothing 13$	180	40	31.5	35	200
$\varnothing 14$	180	40	32.9	35	203
$\varnothing 15$	180	40	33.4	35	204
$\varnothing 16.5$	180	45	37.0	41	204
$\varnothing 18$	180	45	36.7	41	205
Curved					
$\varnothing 11$	230	35	24.6	27	249
$\varnothing 12$	230	35	25.6	27	250
$\varnothing 13$	230	40	31.5	35	250
$\varnothing 14$	230	40	32.9	35	252
$\varnothing 15$	230	40	33.4	35	254
$\varnothing 16.5$	230	45	37.0	41	254
$\varnothing 18$	230	45	36.7	41	254

Unit: mm

Please note that all United Orthopedic Corporation product brochures have been authored in the English language. Any translations into other languages have not been reviewed or approved by United Orthopedic Corporation and their accuracy cannot be confirmed. Any questions regarding United Orthopedic Corporation products should be directed to United Orthopedic Corporation at unitedorthopedic.com/contact.

The CE mark is valid only if it is also printed on the product label.

